



Glover et al.
USSN:
Filed:

Mark Joy
Leydig, Voit & Mayer

Sheet 1 of 3
09/869,637
01/15/02
(312) 616-5600
Ref. # 218499


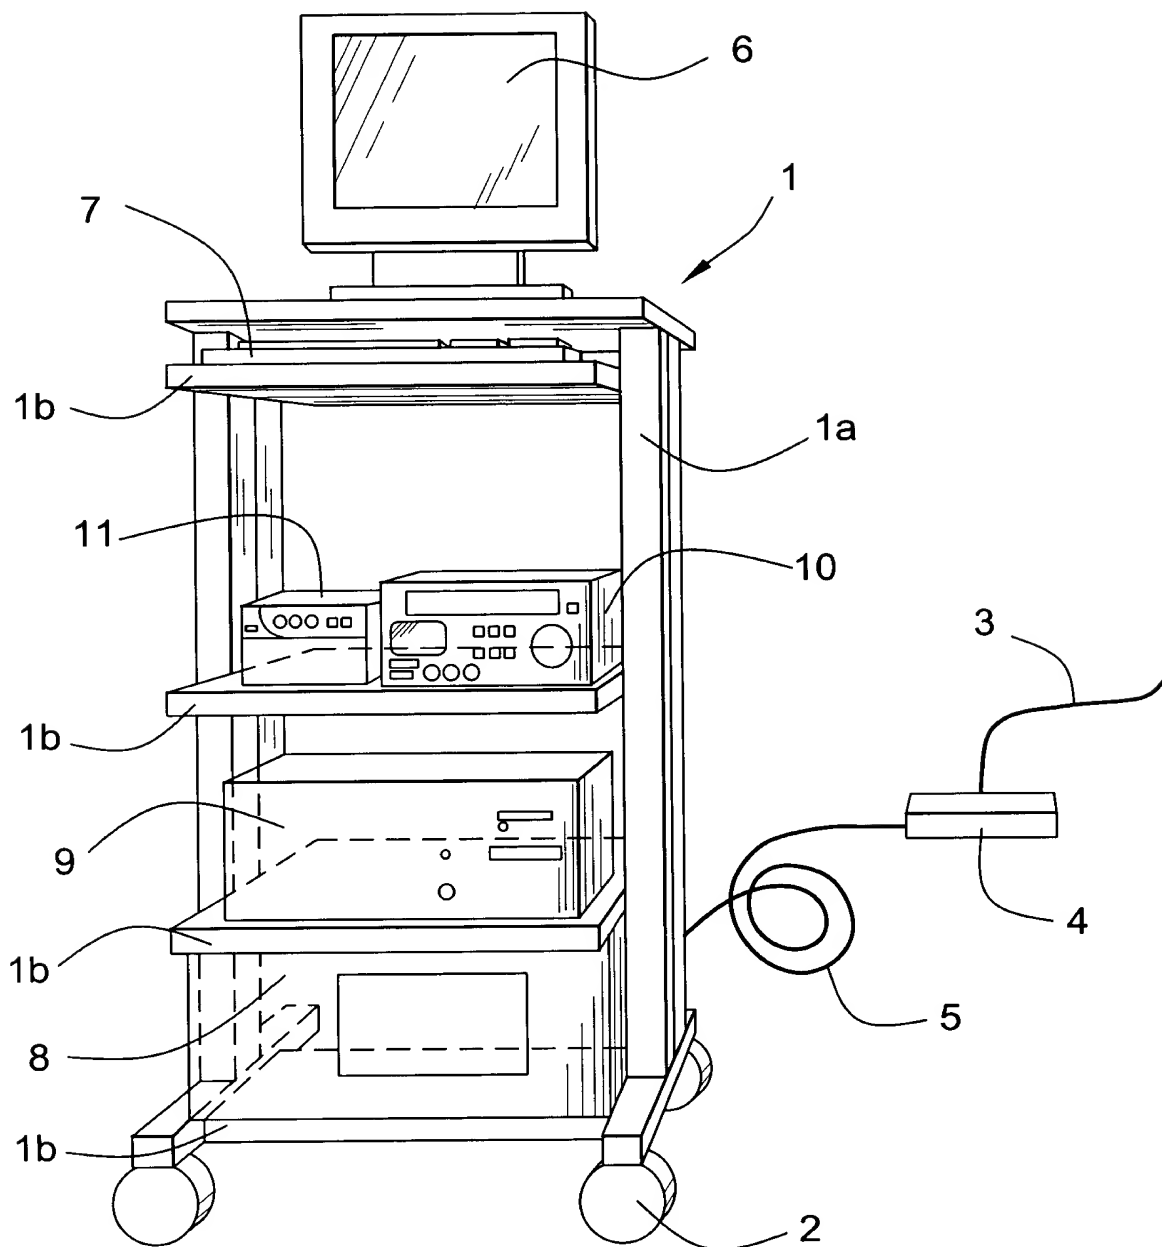



FIG. 1
(PRIOR ART)



A perspective view of a mobile phone 4. The phone has a rectangular body with a display 12 on the front face. The display shows a simple line drawing of a landscape with diagonal lines. A cable is connected to the bottom of the phone.

A schematic diagram of an IVUS system in an X-ray room. The diagram shows a patient lying on a table (4) with a catheter (12) inserted into a blood vessel. A control console (9) is connected to the catheter via a cable (15). A monitor (13) displays the IVUS image. A stand (14) holds a probe (16) and a control unit (17). A key IVUS specific component is shown at the bottom.

FIG. 3

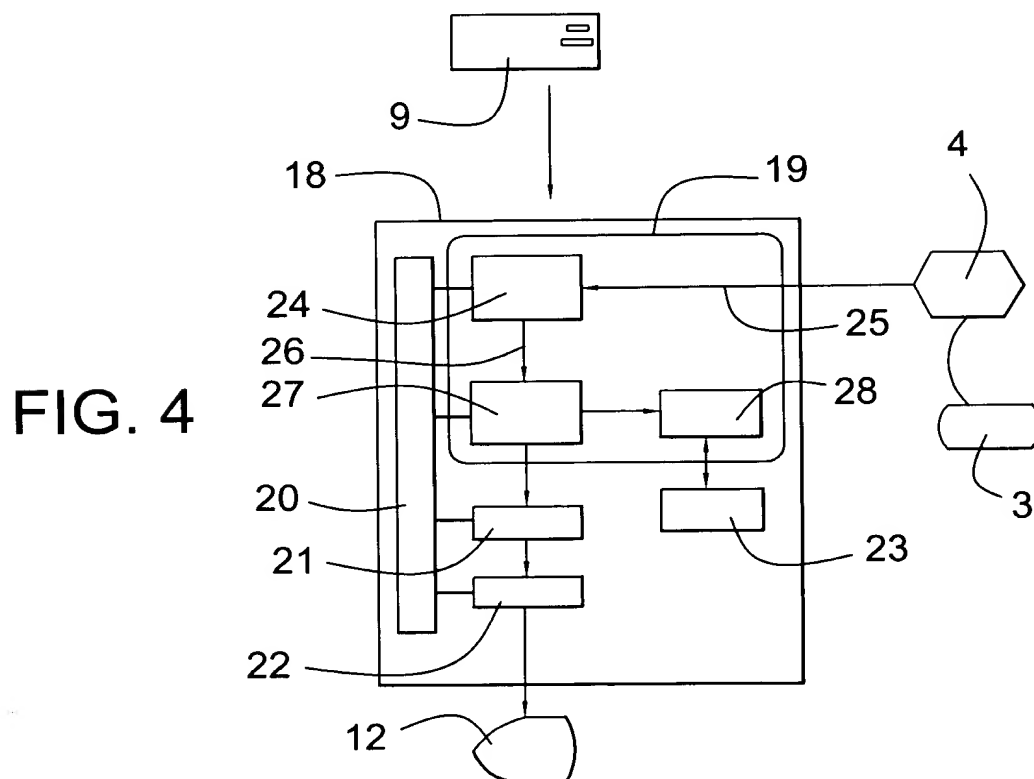

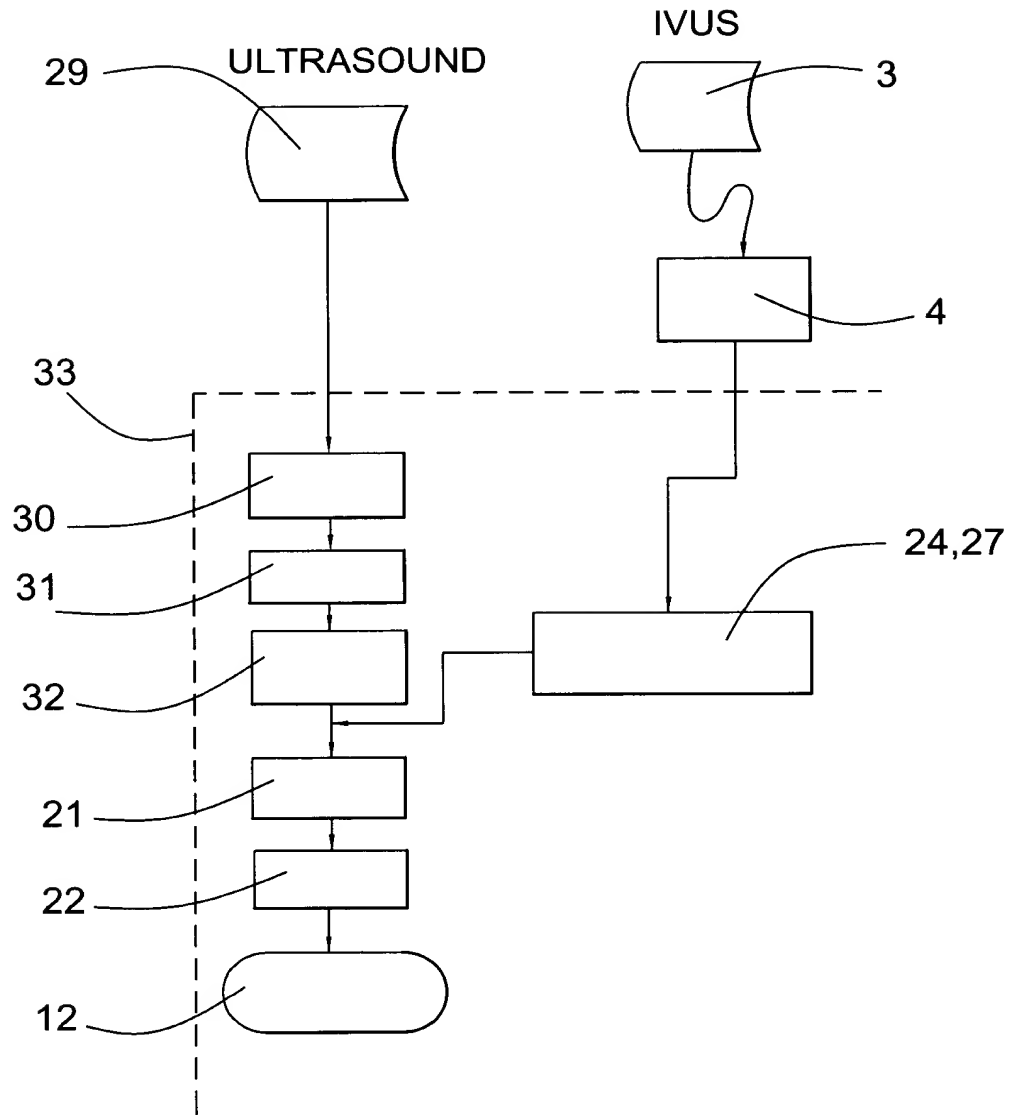


FIG. 5